
Quick Start Instructions

1. Insert 9V Battery


System comes with factory setings: Full Volume and Tone 1.



Note: Black ribbon goes underneath battery for easy removal.

2. Push "Learn" Button

Alarm will beep 3 times

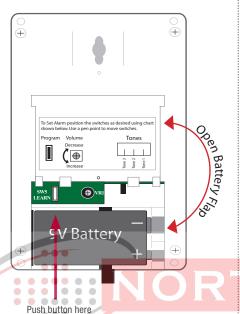

3. Plug in Transmitter

You now have 30 seconds to plug in transmitter to cord coming out of pad. Switch Transmitter On/Off button to "On". Alarm will make one long beep and is now programed. Close neck of pad with button snaps. (Also see instructions on pad).



SAFETY

4. Test System



Apply pressure to pad to activate alarm. 2 beeps indicates alarm is functioning.

Alarm will sound when pressure is released from pad. Press "reset" button on front of monitor to silence alarm.

"Status/In Use" light blinks only when pad is plugged into monitor and pressure is on pad.

5. Mounting Options



Drill hole into headboard or wall.


Hang monitor on screw using mounting hole on back of monitor.



Note: Other mounting options available. Call 800.650.3637 for more information.


Adjust Settings (Optional)

System comes with factory settings: full volume, tone 1. Use a small flathead screwdriver to adjust volume and a pen point to adjust tones.

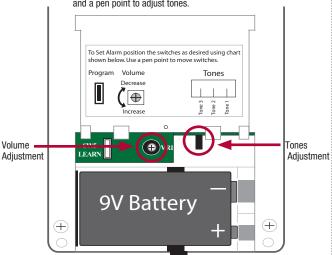

Tamper Proof/Caregiver Key Mode

Use Caregiver Key to allow only the Caregivers to silence the alarm! This will cancel the function of the "Reset" button.

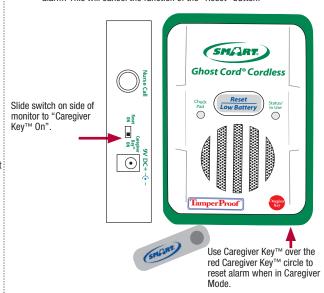













monitor will blink when pressure is applied to pad.

silence the alarm. The status light on the front of

pad. Press "reset" button on front of monitor to

Alarm will sound when pressure is released from

Apply pressure to pad to activate alarm. Monitor will

mounting locations include: back of headboard, back Place monitor out of reach of resident. Suitable

Wheelchair Pressure Pads

monitor will blink when pressure is applied to pad. silence the alarm. The status light on the front of pad. Press "reset" button on front of monitor to

Alarm will sound when pressure is released from

Apply pressure to pad to activate alarm. Monitor

Place pad under lower back/buttocks to be alerted

Place pad under shoulders to be alerted when

will beep twice when active.

when resident vacates the bed.

beep twice when active.

Center pad under buttocks.

WHEELCHAIR/CHAIR PLACEMENT

of wheelchair, wall or under bed.

TEST SYSTEM



OTHER DAMAGES ARISING OUT OF THE USE OF THE GOODS.

AGES TO REFUND OF THE PURCHASE PRICE OR REPLACEMENT OF THE GOODS. SELLER DISCLAIMS ANY LIABILITY FOR COMPENSATORY OR WHERE PERMISSIBLE, IT IS THE SELLER'S INTENT TO LIMIT ANY LIBBILITY FOR SPECIAL, CONSEQUENTIAL OR INCIDENTAL ECONOMIC DAM-

c.) Testing of the system before each use.

b.) Adequate training for staff personnel for elopement

a.) Direct patient supervision

including, but not limited to:

the buyer to insure that the system is properly installed and tested. Further, the system is not designed to replace good care giving practices The Smart Caregiver Corporation GHOSTCORD® monitors are designed to be installed by the end-user. As such, it is the entire responsibility of

ob retailer, assumes the entire cost of all necessary installation, servicing or repairs. THE BUYER. SHOULD THE GOODS PROVE DEFECTIVE FOLLOWING THEIR PURCHASE, THE BUYER, AND NOT THE MANUFACTURER, DISTRIBUTOR CHASED ARE BEING SOLD ON A "WITH ALL FAULTS" BASIS. THE ENTIRE RISK AS TO THE QUALITY AND PERFORMANCE OF THE GOODS IS WITH Warranties are given and no affirmation of seller, by words or action, will constitute a warranty. The goods being pur-Other than this limited warranty, seller makes no express or implied warranties. Except for this limited warranty, NO EXPRESS OR IMPLIED Seller warrants that the goods sold will be free from defects of workmanship and manufacturing, for a period of one year from the date of sale.

Test this device before each use. Read the instructions and Legal Disclaimer.


and or stop falls. This device is to help augment caregivers comprehensive resident mobility management program. required. This device is not a substitute for visual monitoring by caregiver. The manufacturer does not claim that this device will stop elopement Warning: Failure to comply with warning may result in injury or death. This device is not suitable for all individuals. Other devices may be

TL-2100G Ghostcord Cordless® System

Installation Instructions

TL-2100G Ghostcord® Cordless Monitor

BED PLACEMENT

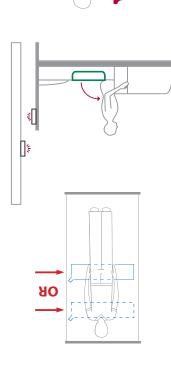







TEST SYSTEM

resident sits up in bed.

Place pad under sheet.